

## Model 751537-E2 RACK MOUNTING KIT for FG400 (Single-housing Rack, Inch type)

### 1. Checking the Parts in the Kit


Confirm that all parts listed below are included in the kit. If any part is shorted or any abnormality is found in the appearance of the parts, contact our sales representative where you bought the instrument.

List of parts included in the kit.

Right side bracket (1 pc), left side bracket (1 pc), flat-head screws (M3, 10 mm long) (4 pcs)

### 2. Removing the Parts from the Instrument


1. Remove the four feet.
2. Remove the two sealing labels.

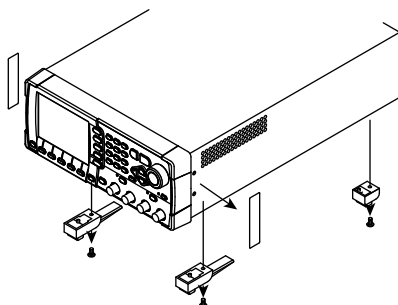

### 3. Joining the Instruments with Mounting Hardware

1. Using two flat-head screws (M3, 10 mm long) (3), screw the right side bracket (1) to the right side and the left side bracket (2) to the left side of the instrument.

Reference torque value: 0.6 to 0.7 N·m

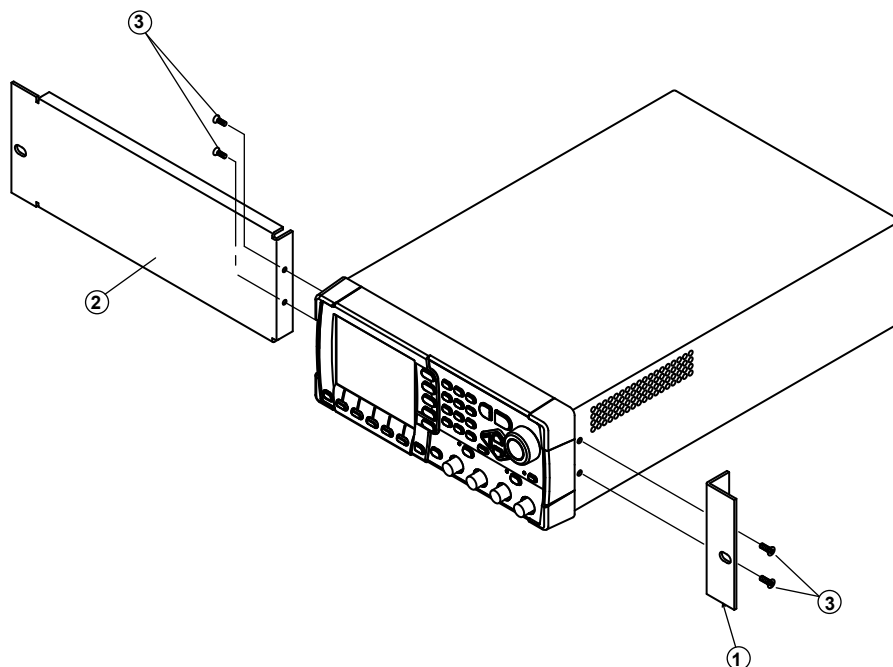

## 5. Mounting the Joined Instruments to the Rack

Dimensions after mounting to the rack are illustrated below.

**Be sure to place support beneath the rack.**

